

Yocom-McColl Testing Laboratories, Inc.
 540 West Elk Place • Denver, Colorado 80216-1823 USA
 PHONE (303) 294-0582 • FAX (303) 295-6944
 EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)
 Micron Test Report**

Alpacas of Kentucky/B.J. & Donna Witherspoon
 332 Vance Lane
 Bowling Green KY 42101

08/05/07


Test No: 304585

Animal and Sample Description

Animal Name:	ADKY Kentucky Darby	Animal ID:	30500600
Breed:	Alpaca(Huacaya)	Sample Location:	Side
Sex:	Female	Sample Date:	04/11/07
Color:	White	Age:	06/06/06

Laboratory Data

Mean Fiber Diameter:	20.2 microns
Standard Deviation:	3.9 microns
Coefficient of Variation:	19.2 %
Fibers Greater Than 30 microns:	1.7 %

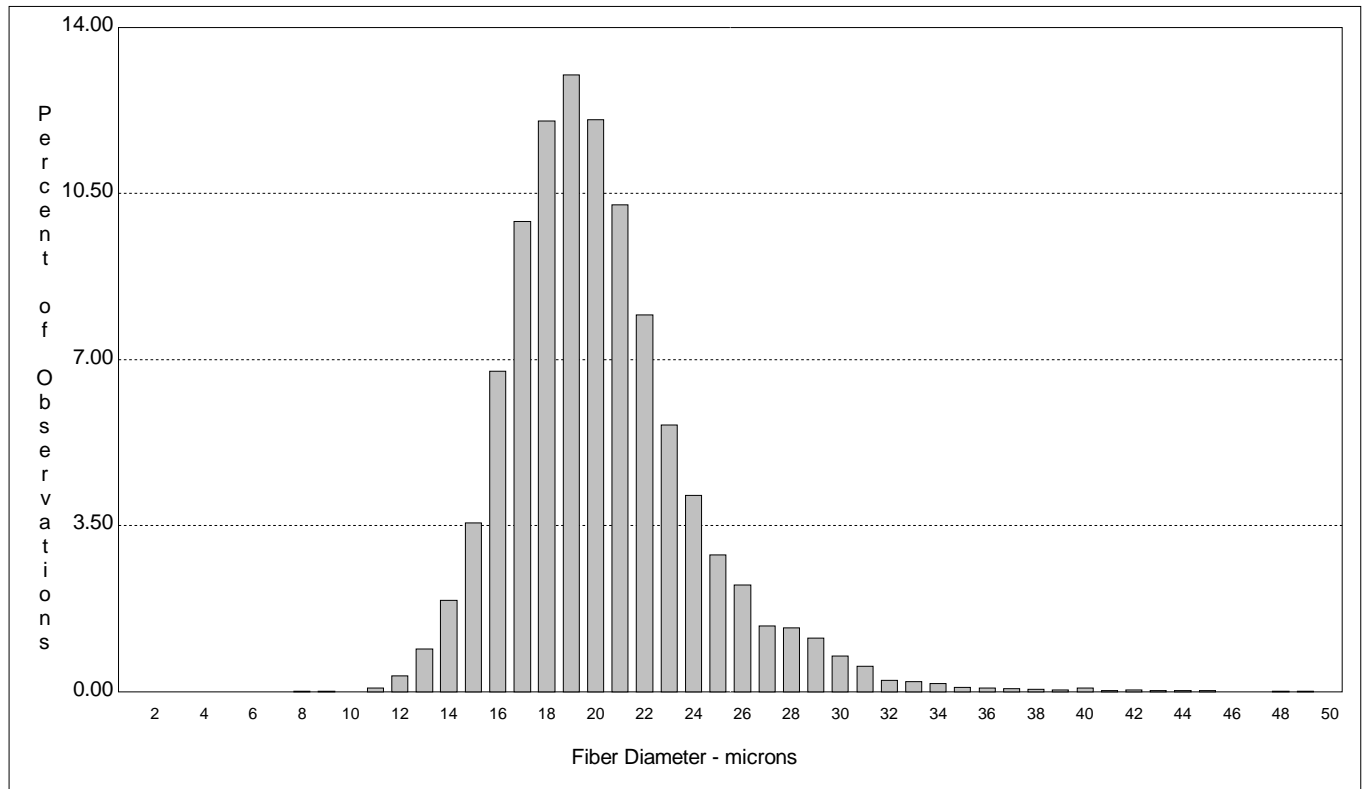

This Test Performed According to I.W.T.O Method 47